

Semi-Quantitative Non-Targeted Analysis as a Rapid Risk Prioritization Tool: *A Proof of Concept Using Activated Carbon Drinking Water Filters*

Louis Groff, Hannah Liberatore, Seth Newton, Jon Sobus



Why Does EPA Need Measurement Data?

- Measurement data needed to assess chemical safety
- Regulate chemicals, manage exposures, ensure compliance under several federal statutes

Federal Insecticide, Fungicide and Rodenticide Act Compliance

Mo
The Federal
gives EPA
sale and
including
Safe Drinking Water Act (SDWA) Compliance Monitoring


Providing sa
states, tribe
certified lab
water samp
the tribes m
Water Act re
Toxic Substances Control Act (TSCA) Compliance Monitoring

To protect human health and the environment, EPA works with its federal, state, and tribal regulatory partners to assure compliance with statutes and regulations in the manufacture (including import), processing, distribution in commerce, use, or disposal of chemical substances. The major federal law governing chemical substances is the Toxic Substances Control Act (TSCA).

Resources and Guidance Documents


- [Compliance Assistance Resources and](#)

Chemical Monitoring Needs

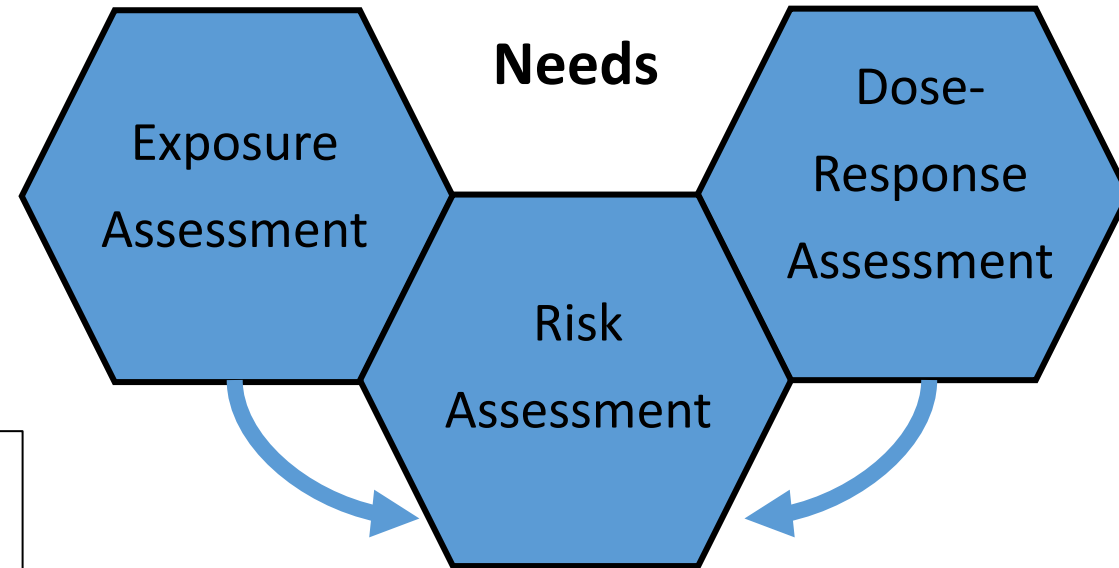


Traditional Targeted Analysis

Purchase standards for quantitation



Different Signal Intensities Across Compounds

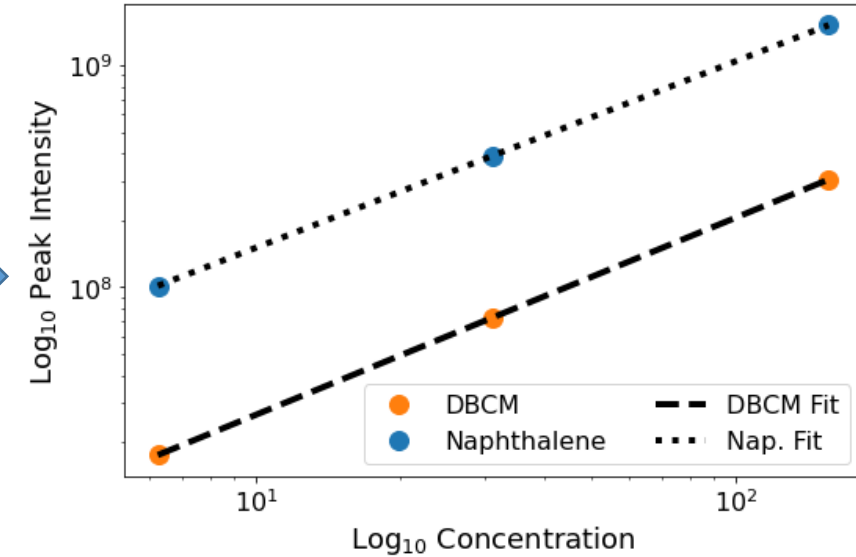

Calibration Curves Allow Accurate Quantification of Individual Analytes

Limitations of Targeted Analysis


- Environmental & biological samples are typically highly complex mixtures
- Contain diverse arrays of known and unknown chemicals (100s-1000s per sample)
- Targeted confirmation/quantitation of all compounds-of-interest not remotely feasible

General NTA Workflow


Samples



High-Resolution MS

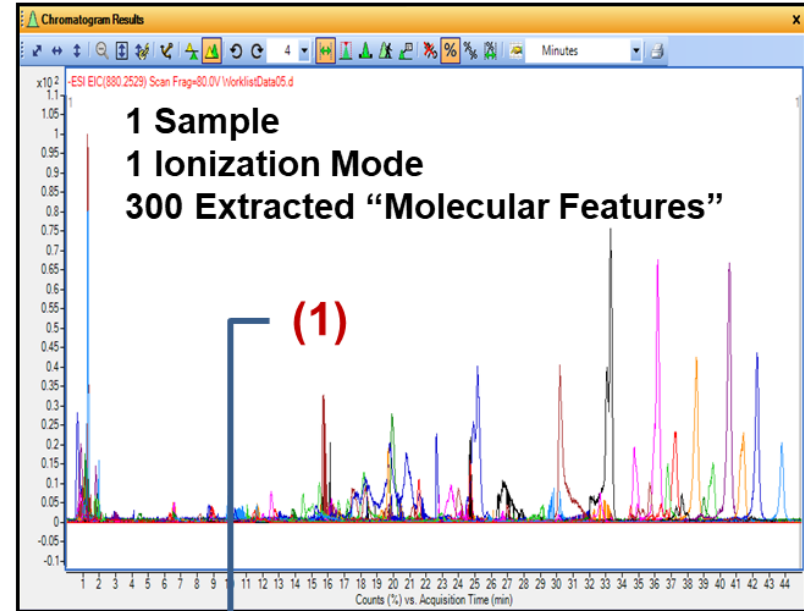

- 1) Prioritize "molecular features"
- 2) Correctly assign formulas
- 3) Correctly assign structures
- 4) Predict chemical concentrations
- 5) Determine chemical sources




Semi-Quant. (SQ) NTA is a Multi-Step Process

Media Sample





Extraction & Cleanup




Prepared Sample




MS Analysis



?



?

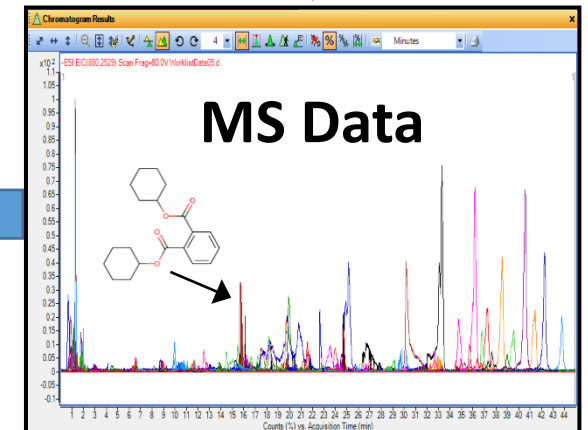


SQ NTA: Need for Rapid Prioritization Methods


- Current SQ-NTA methods have not sought to estimate media concentrations
 - Cannot interpret NTA data in a risk-based context
 - Need ways to defensibly approximate media concentration
- Proof-of-concept approach using GC-HRMS of volatiles in tap water
- Brita filters employed to collect media samples
 - Large-volume water samples (380 L over lifetime of filter)
 - Suitable for low-concentration contaminants
 - Allows preconcentration of analytes on filter
 - Low shipping costs




GC-HRMS Instrumental Parameters

- Electron ionization (EI) source
- Orbitrap mass analyzer
 - Acquisition range: 40-550 m/z
 - *Volatile range observable by GC*




- 
- Split Injection
 - PTV (programmable temperature vaporizing) inlet
 - 60 °C Ramped at 10 °C/s to 290 °C for transfer

- 
- TG-5SiIMS capillary column
 - Oven temperature program
 - 35 °C Ramped at 10 °C/min to 295 °C

Identifying Chemicals: NTA Data Processing Workflow

- Thermo TraceFinder GC-MS Deconvolution plug-in
- NTA approach to detecting compounds
 - Accurate mass tolerance: 5 ppm
 - S/N threshold: 10:1
 - TIC intensity threshold: 500,000
 - Ion overlap: 99%
- Compound identification and RT alignment across samples
 - NIST 2017 EI-MS reference library
 - Results filtered to include only peaks with assigned *mainlib* library matches
 - Reverse search index (RSI) score: ≥ 800
 - High-resolution filtering (HRF) score: ≥ 85
 - Total score: ≥ 85

66/73 compound IDs (standards)
 35/73 compound IDs (extracts)*
 *matrix effects

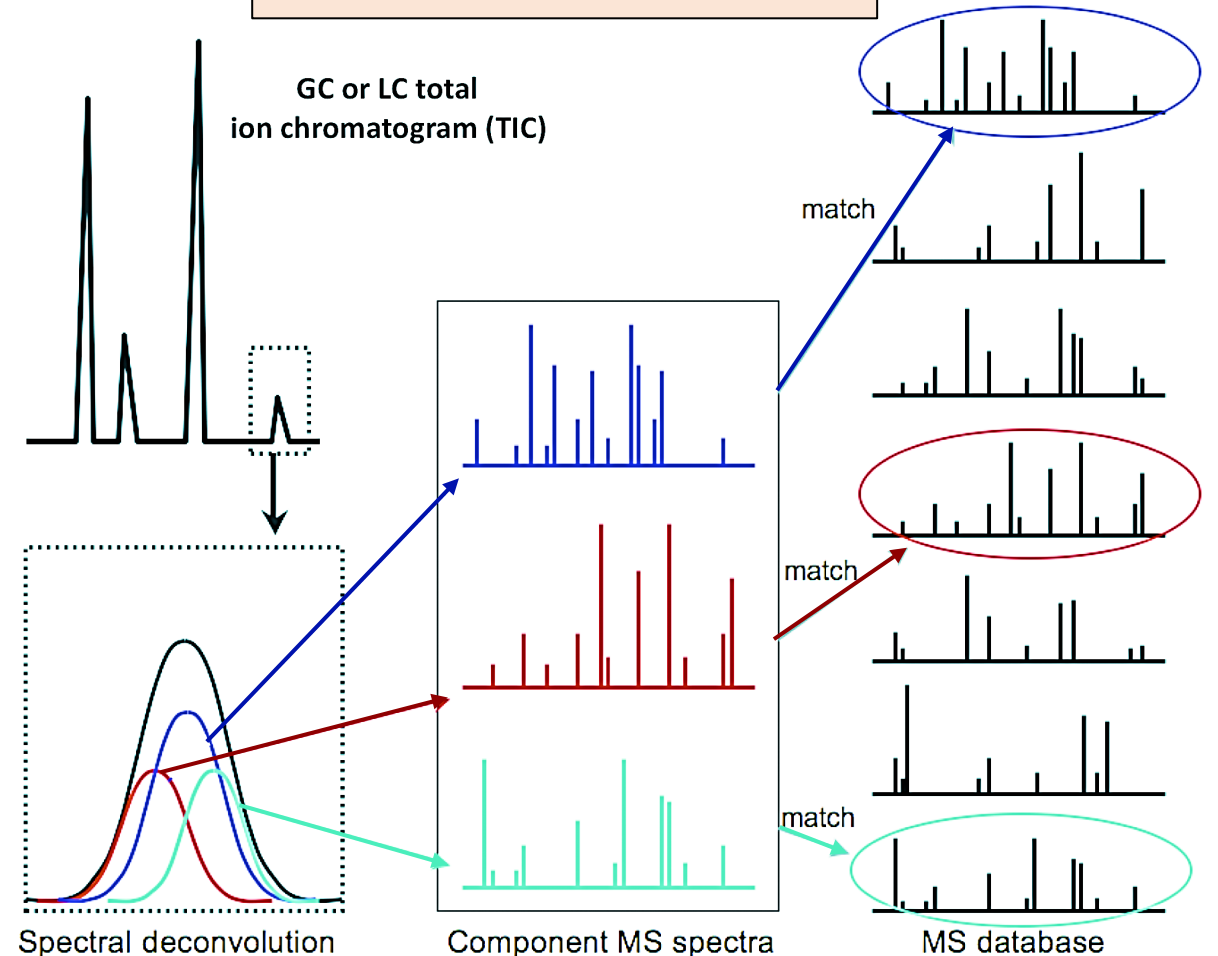


SQ NTA is a Multi-Step Process

Media Sample





Extraction & Cleanup




Prepared Sample




MS Analysis




?



?

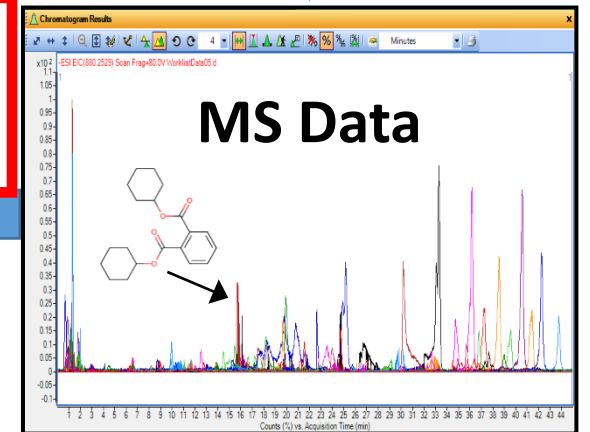

Building a Simple SQ Model Using a Single Surrogate Response Factor

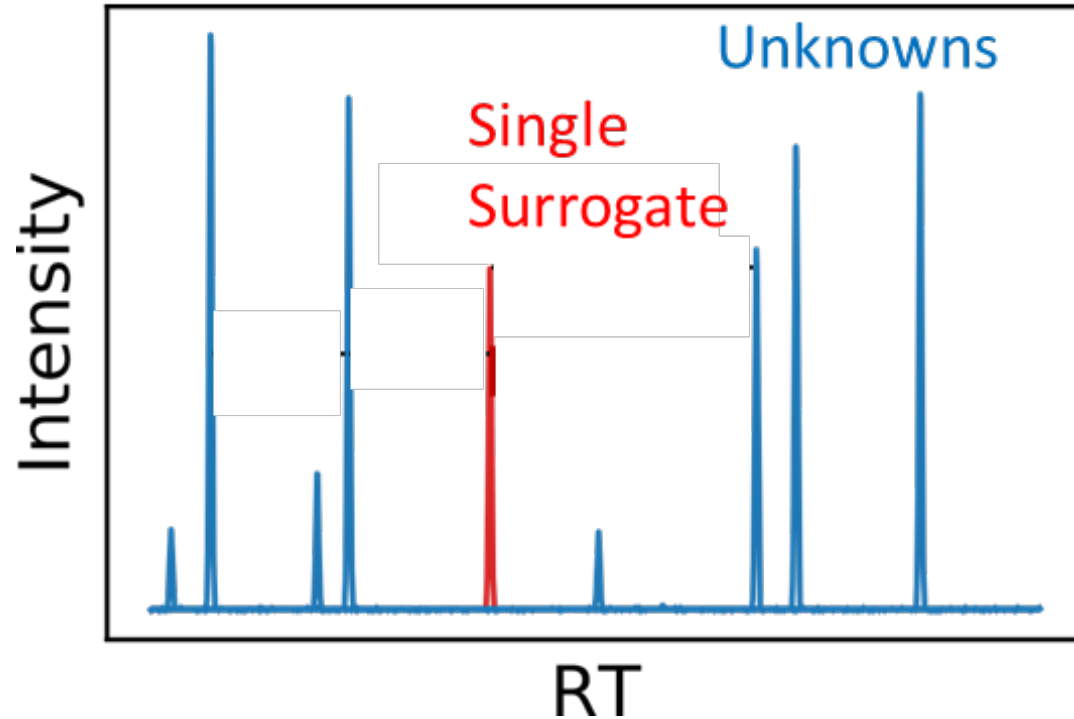

“Single Surrogate” → known chemical spiked at known conc. with observed intensity


“Unknowns” → tentatively identified chemicals with unknown conc. and observed intensities

$$\text{Response Factor (RF)} = \frac{\text{Known Conc.}_{\text{surrogate}}}{\text{Obs. Intensity}_{\text{surrogate}}}$$



$$\text{Predicted Conc.}_{\text{Unknown}} = \text{Obs. Intensity}_{\text{Unknown}} \times \text{RF}$$

Prediction Error Using Single Surrogate Response Factor

- $Error\ Ratio = \frac{Predicted\ Conc.}{Known\ Conc.}$
- Using a single surrogate results in error ratios that span around two orders of magnitude
- Using this SQ approach, we can underestimate by an order of magnitude or overestimate by an order of magnitude




Building a More Complex Model: Relationship Between Intensity and Retention Time

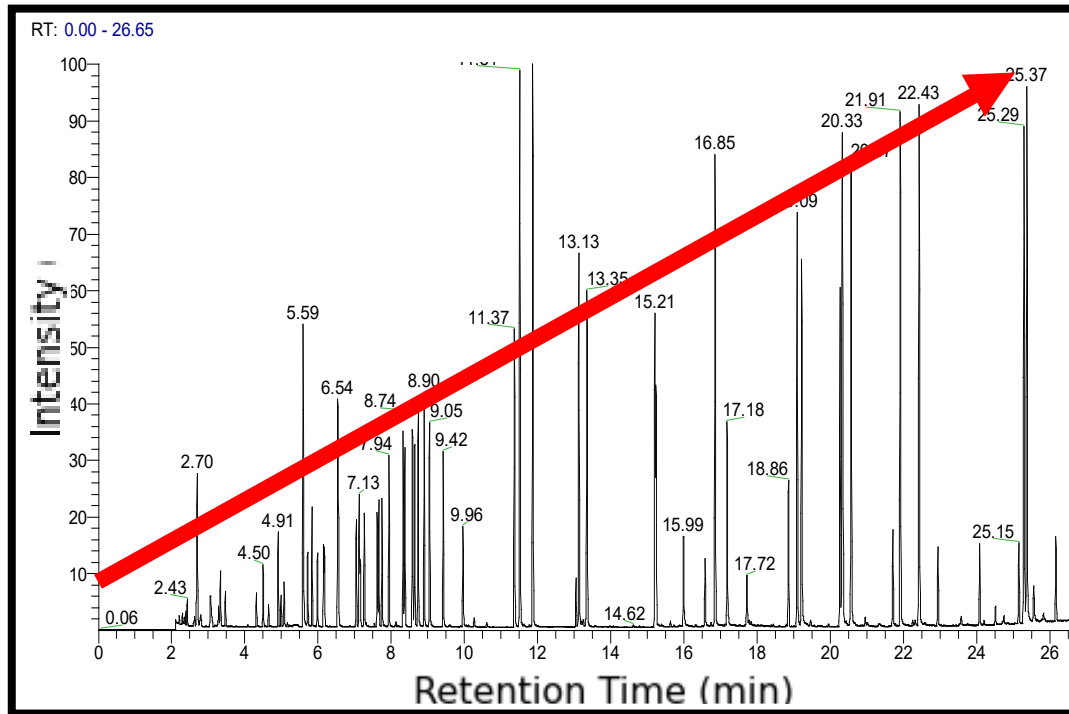

- Found that Intensity Increases as Retention Time Increases at the same concentration
- Can utilize to improve model predictions

Building a More Complex SQ Model

Use to bound Concentrations According to Absolute Retention Time Difference

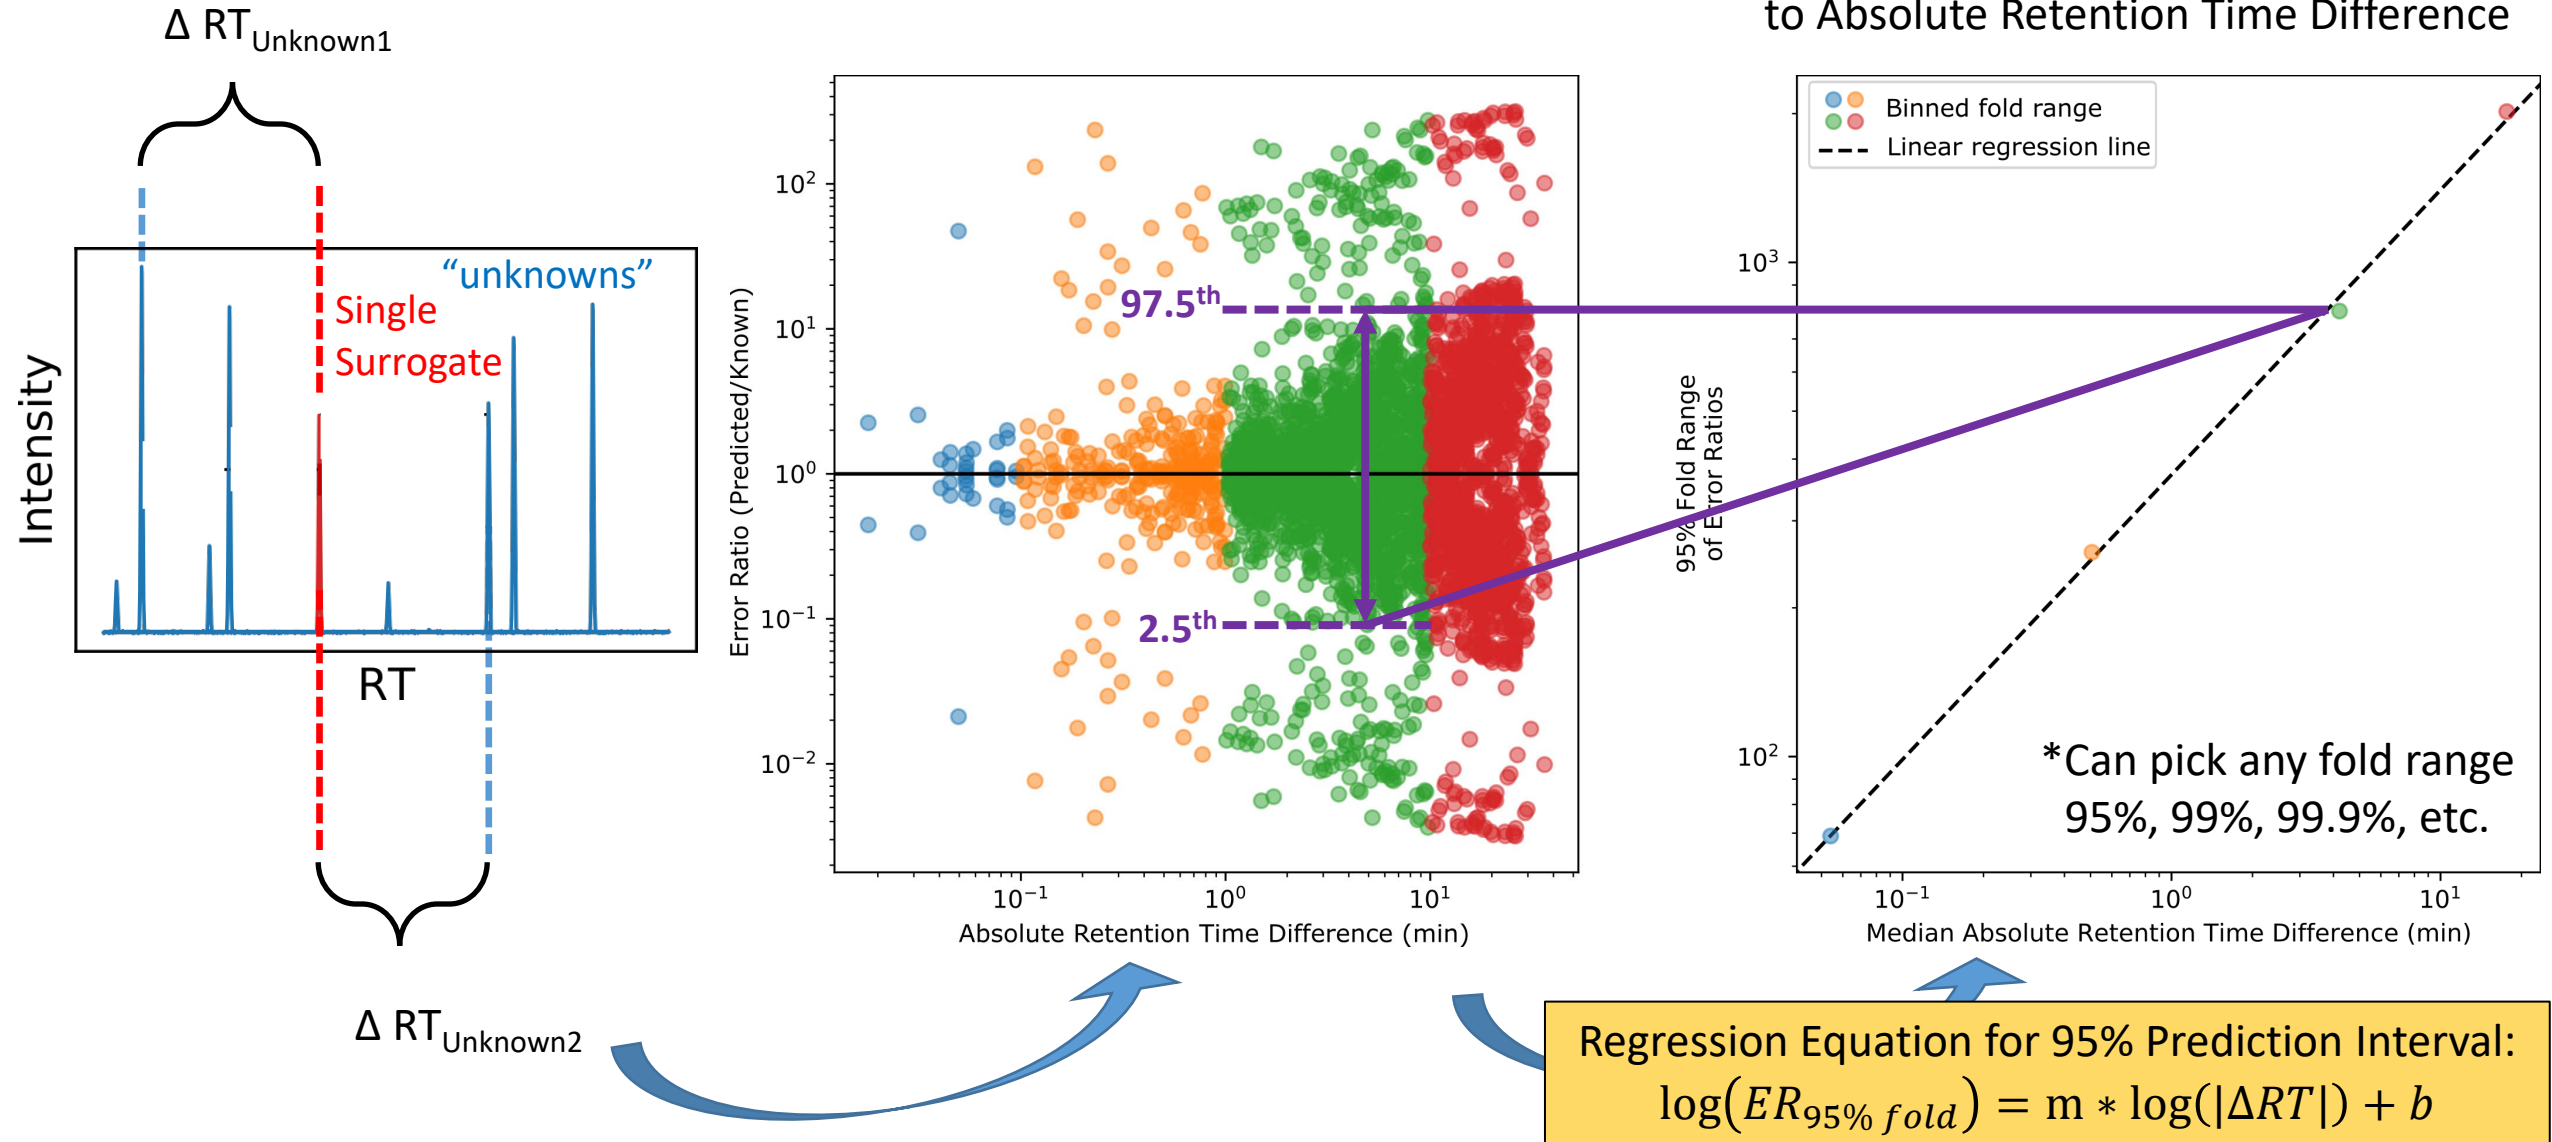


*Can pick any fold range
95%, 99%, 99.9%, etc.

Regression Equation for 95% Prediction Interval:

$$\log(ER_{95\% fold}) = m * \log(|\Delta RT|) + b$$

Implementing the Model for Prediction (Step 1)

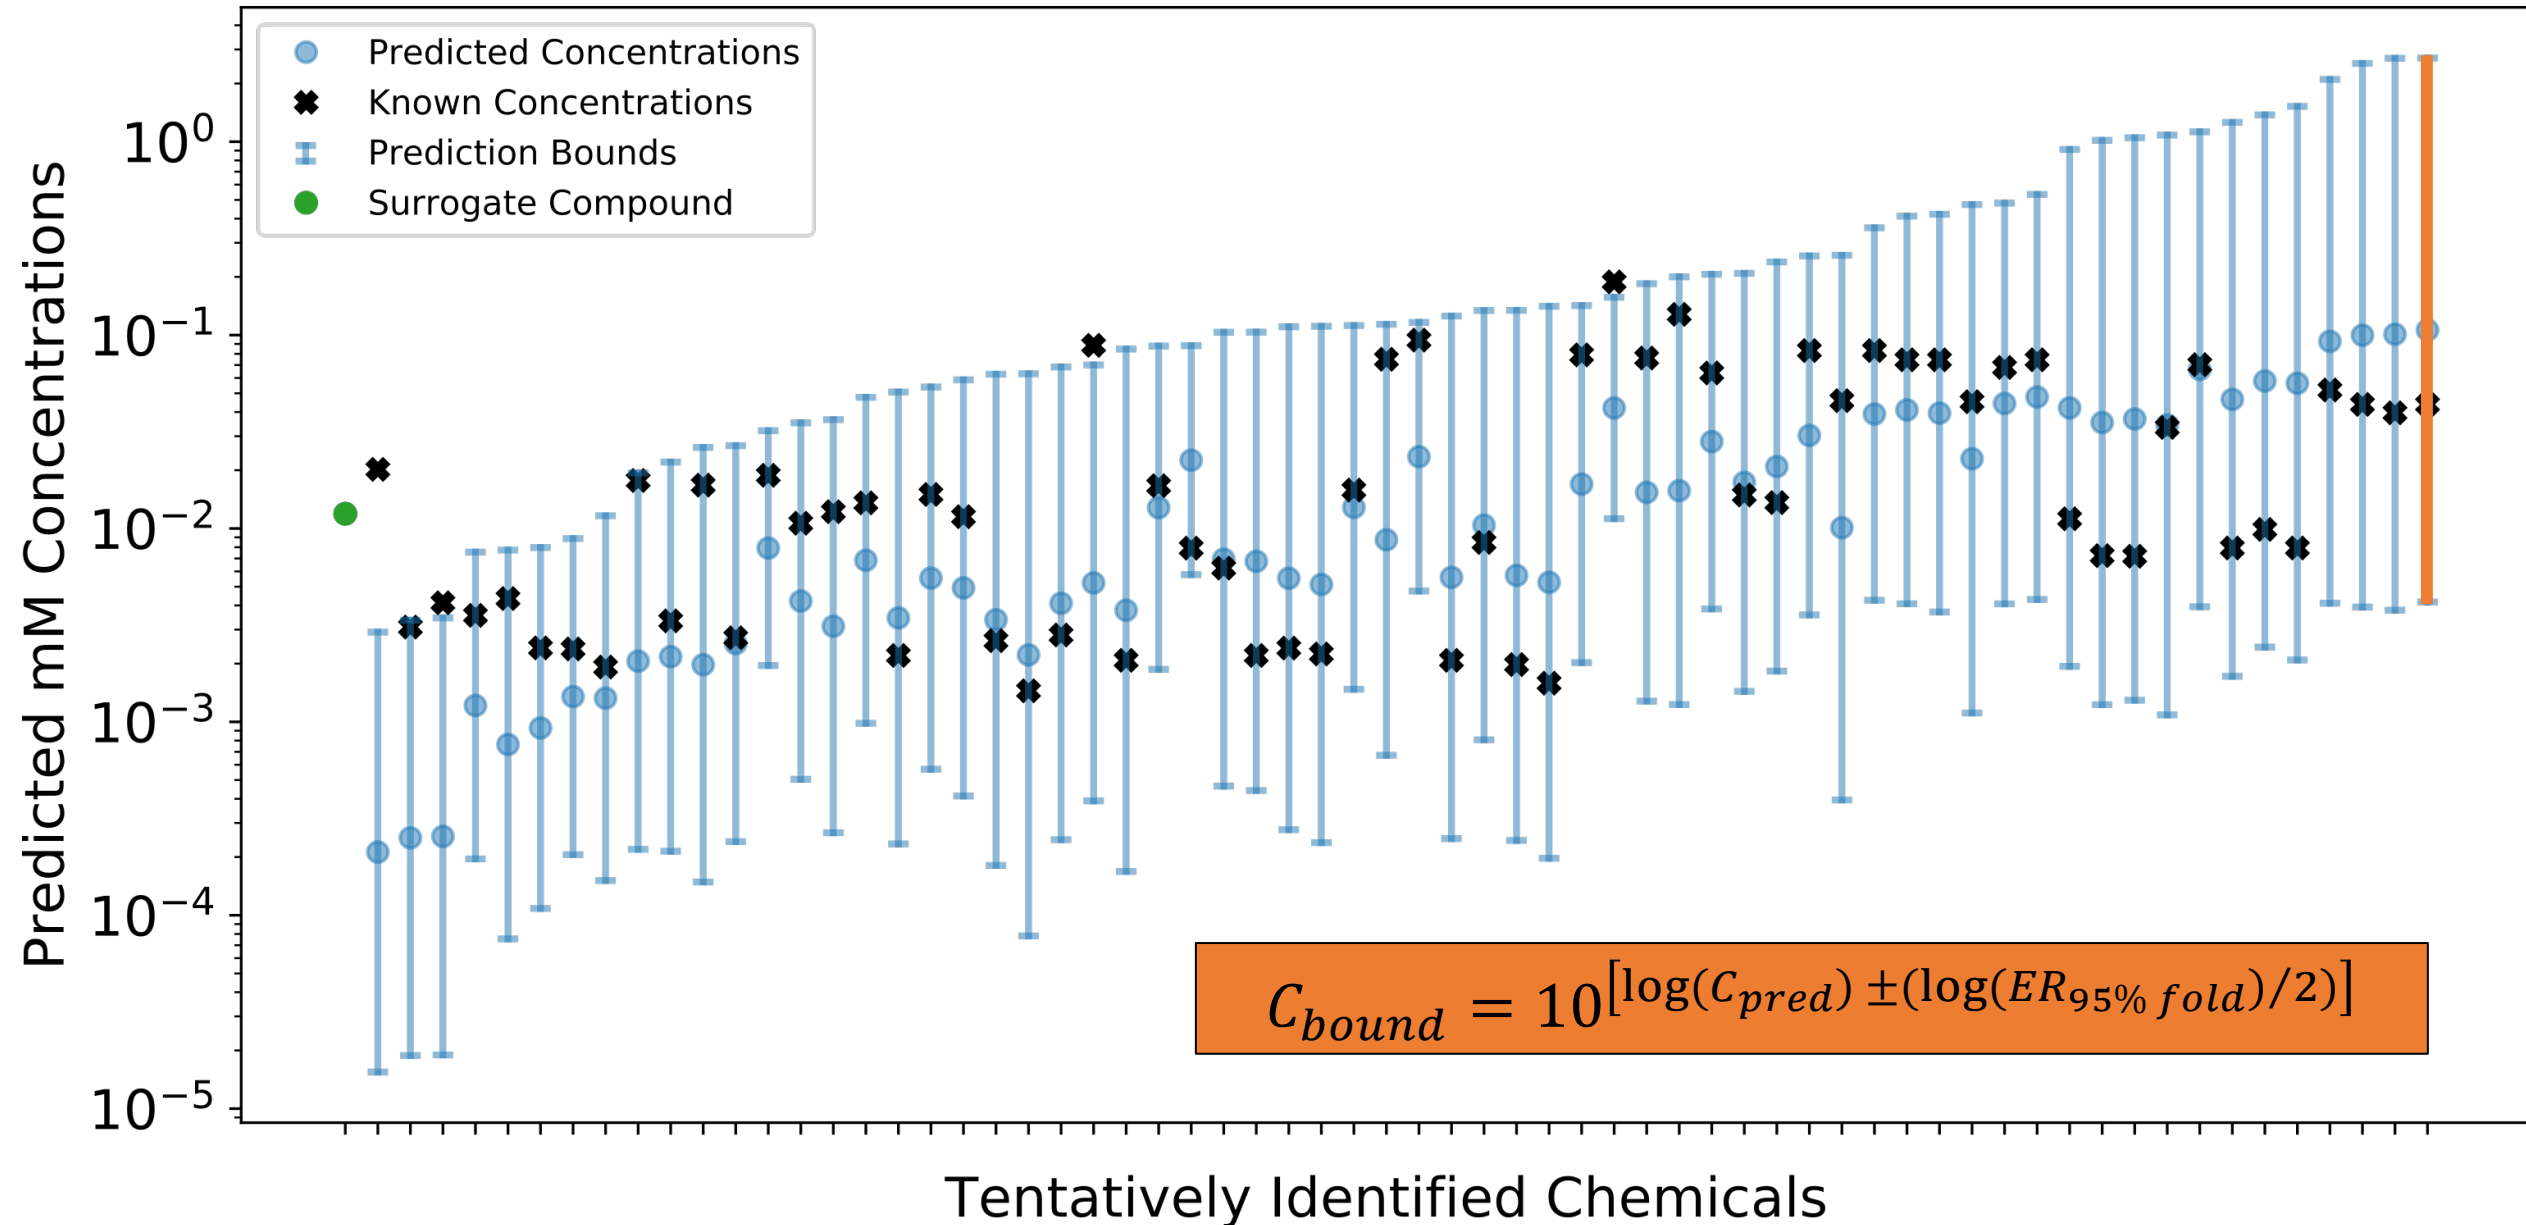


SQ NTA is a Multi-Step Process

Media Sample







Extraction & Cleanup



Prepared Sample




MS Analysis

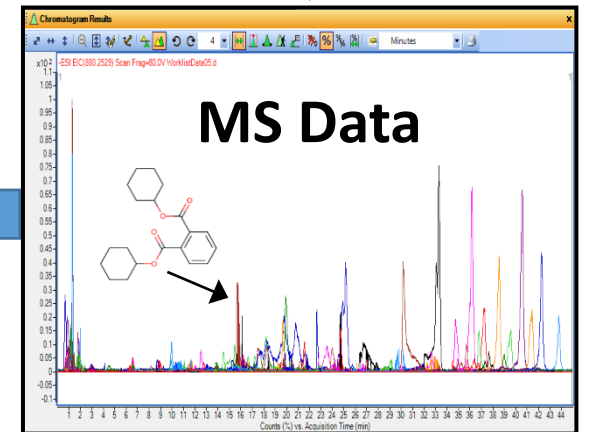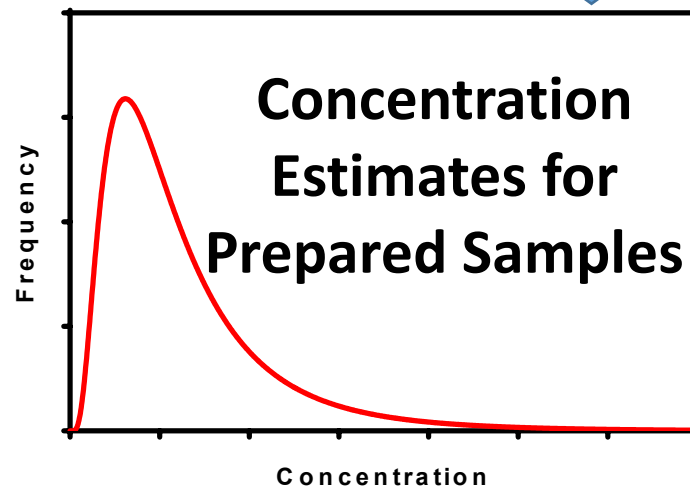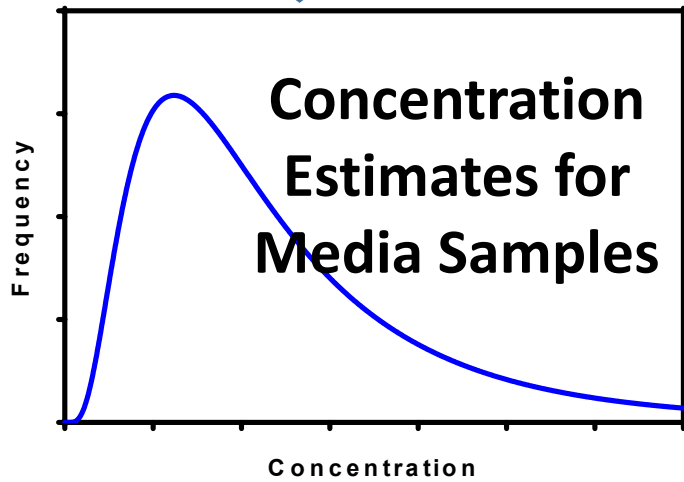


Why is "Recovery" a Critical Parameter?


Max. Percent Recovery = 100% → known lower bound on media conc.
 Min. Percent Recovery = ?% → no upper bound on media conc.



Upper Bound
Solution Estimates




Percent Recovery
From Media



Media Estimates

Example Prioritization Using Tap Water Filters

From Brita Extracts

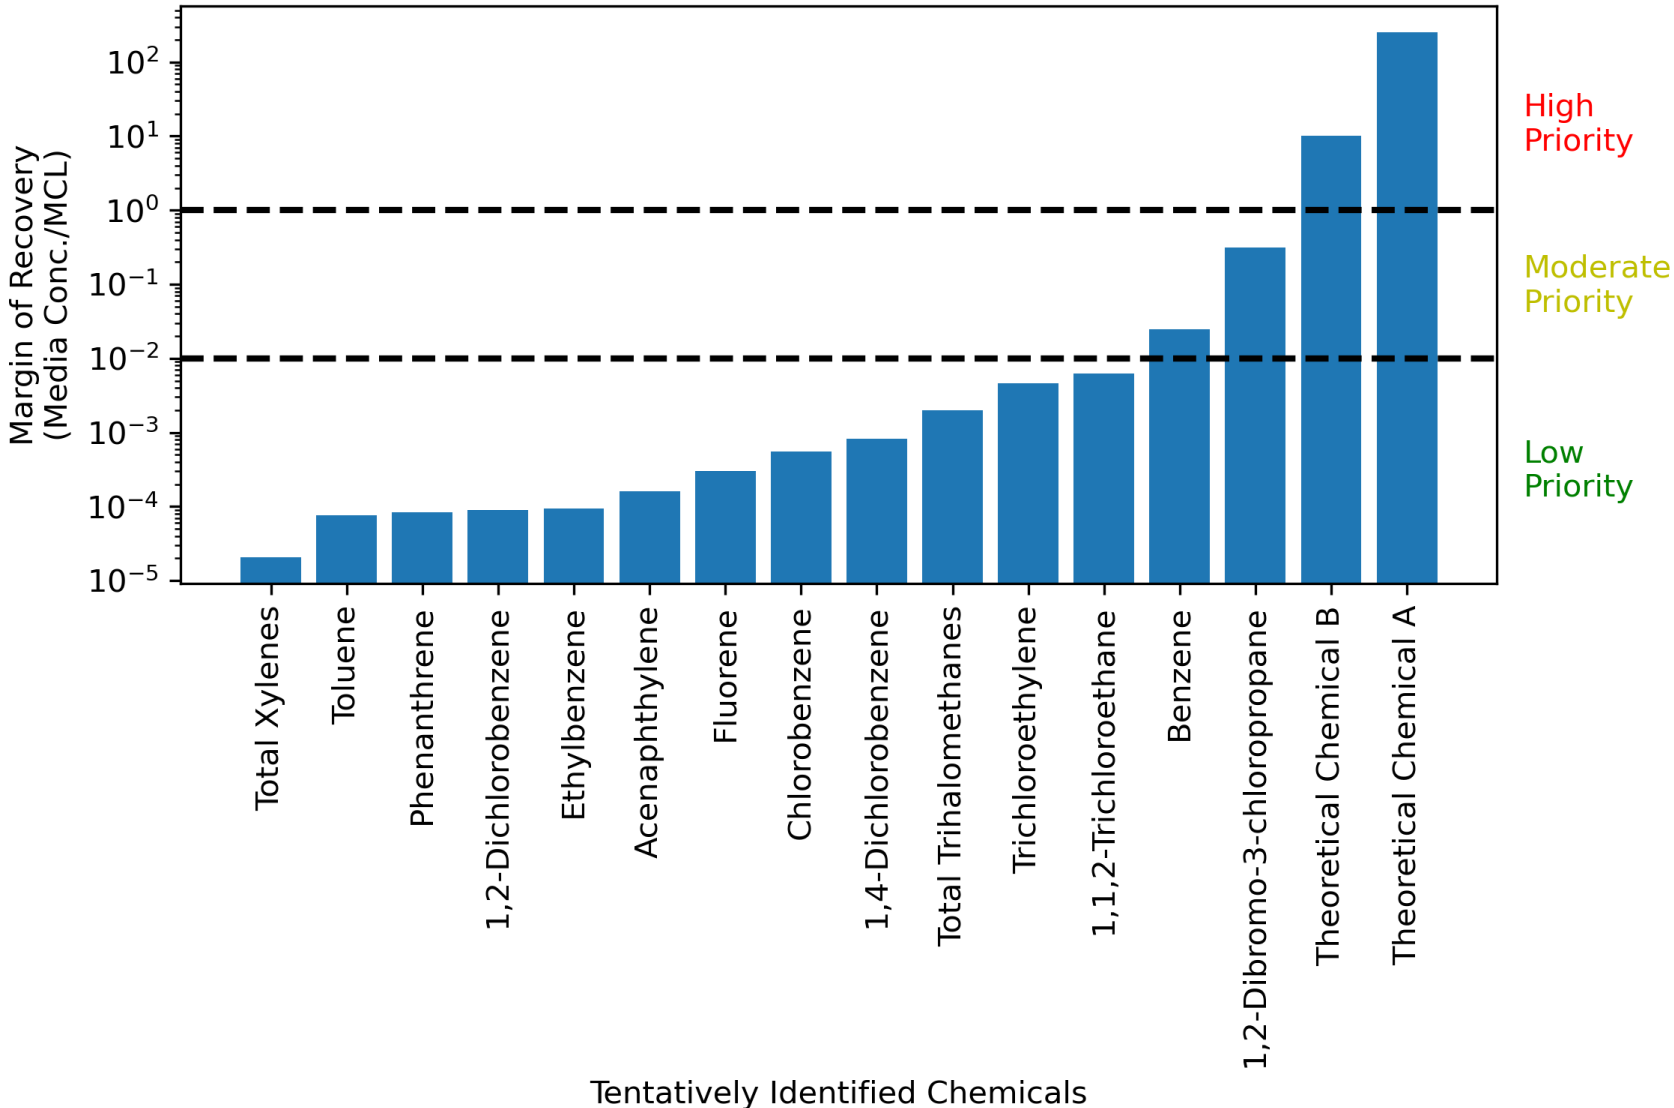

Prepared Solution Conc.



Media Conc.

Adjust by concentration factor


$$\text{Conc Factor} = \frac{\text{Vol. Filtered Tap Water}}{\text{Vol. Extract}}$$

Compare to EPA

Max Contaminant Levels (MCL)

Example Prioritization Using Tap Water Filters

From Brita Extracts

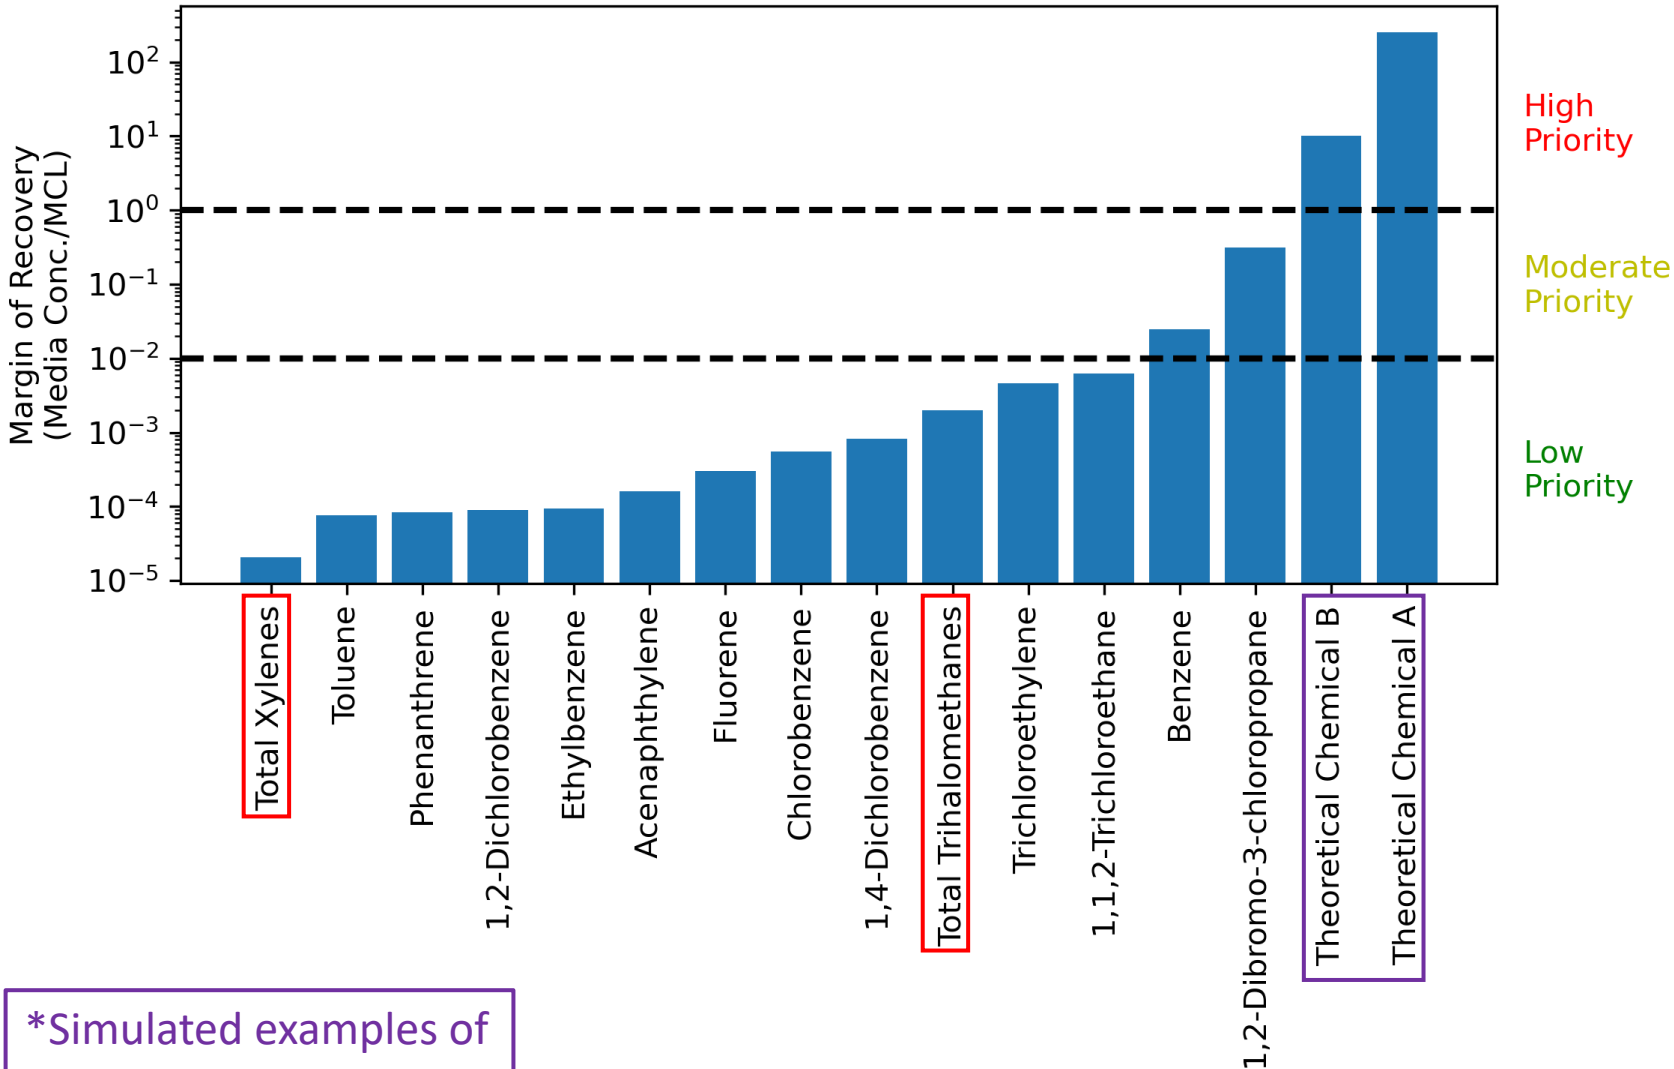

Margin of Recovery (MoR)
Calculated for risk prioritization

$$MoR = \frac{Upper\ C_{media}}{MCL} \times 100$$

Priority Levels:

Low → MoR < 1%

Moderate → 1% ≤ MoR < 100%


High → MoR ≥ 100%

Moderate & High priority
candidates for targeted analyses

*Simulated examples of
high-priority chemicals

Tentatively Identified Chemicals

Conceptual Model for Interpretation

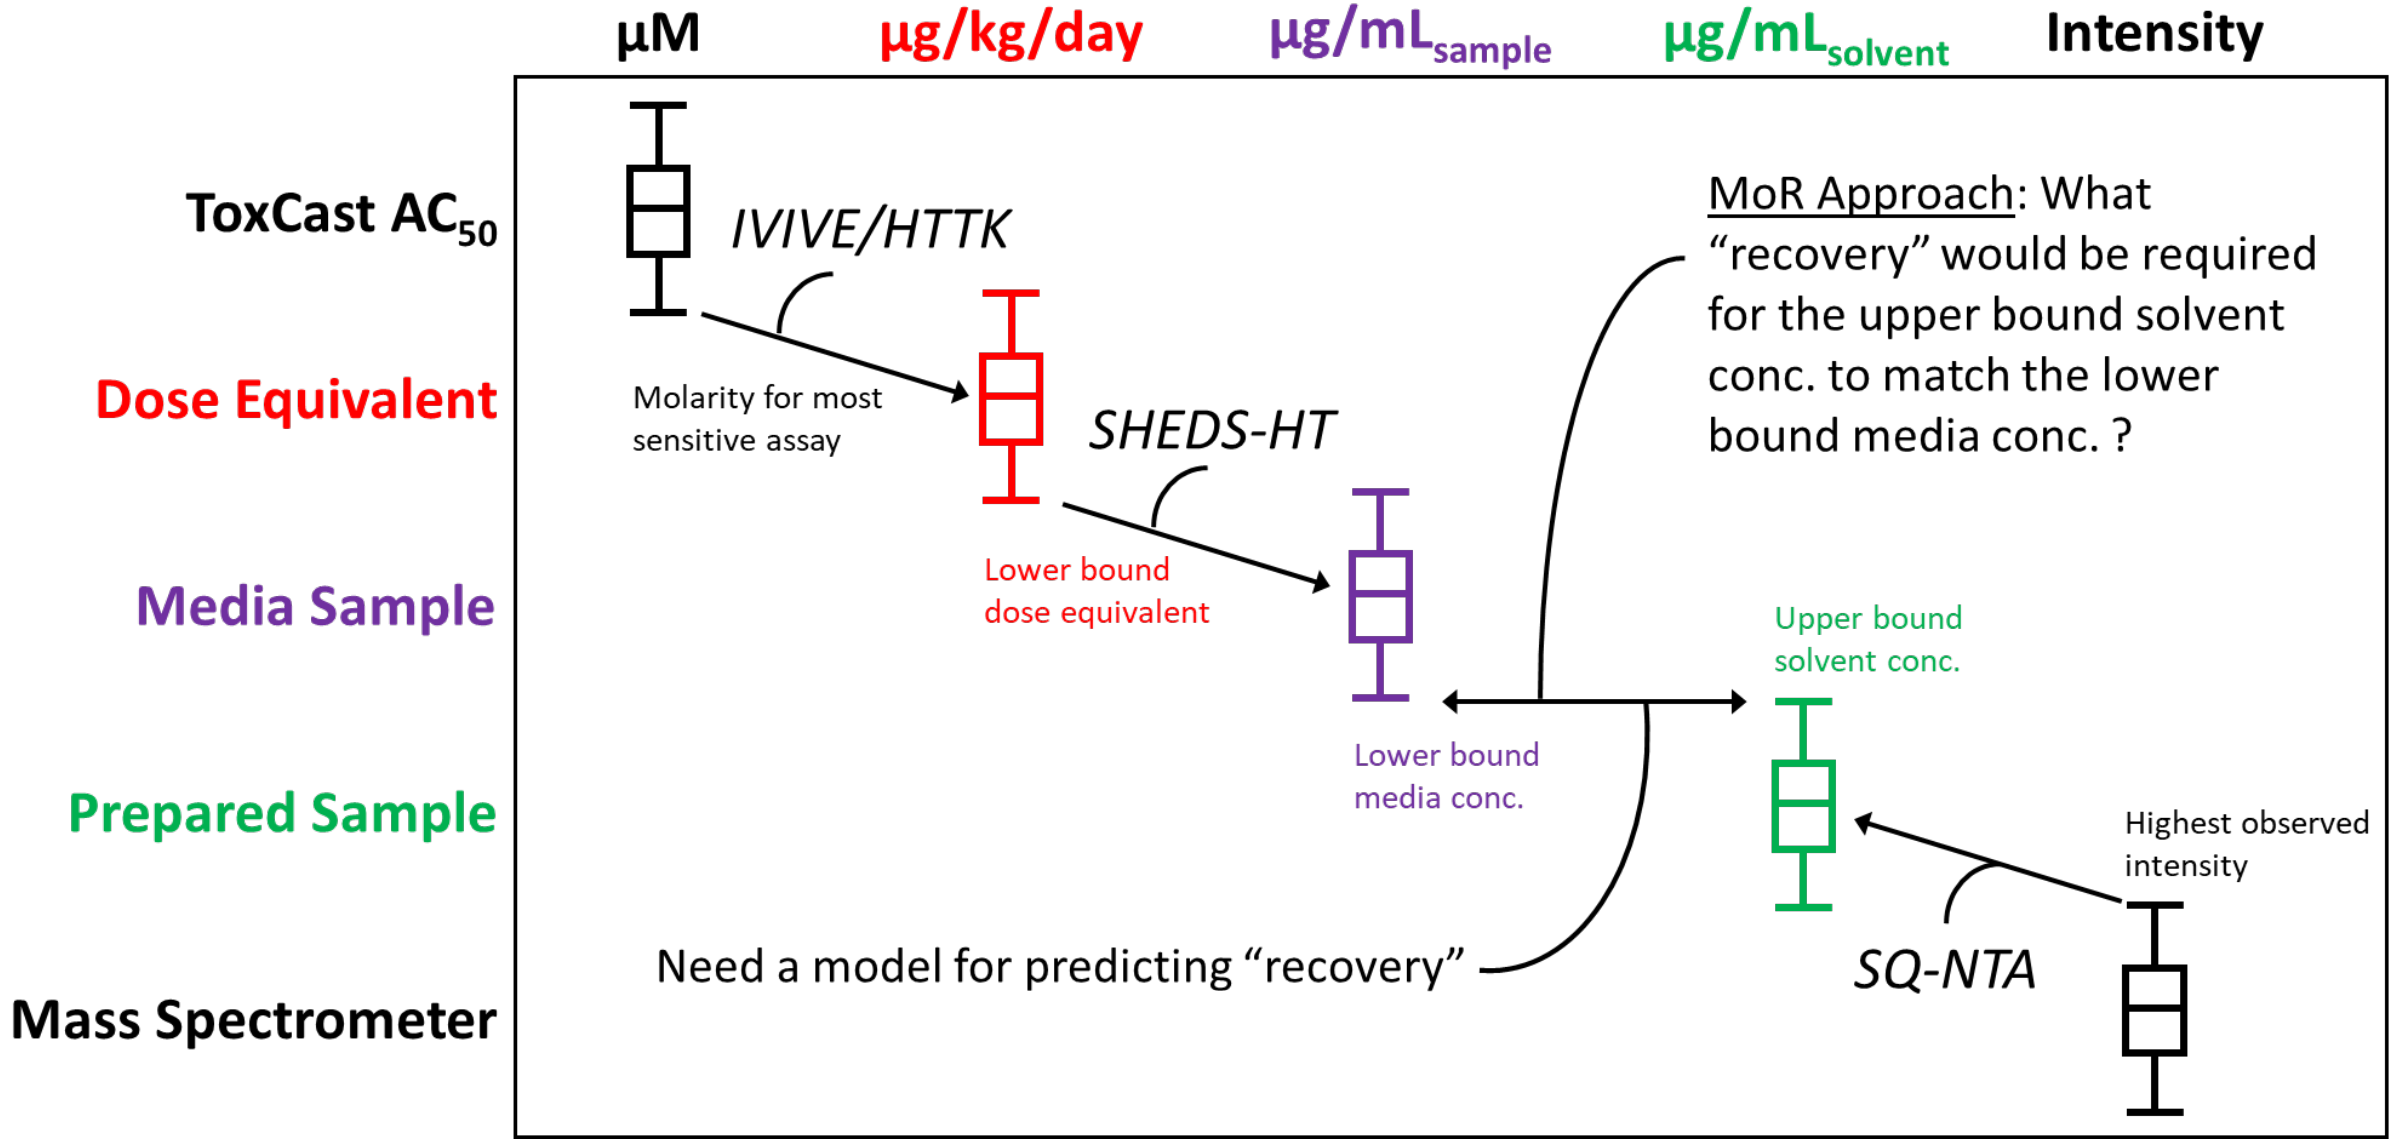

Planned Activities

- Finalize semi-quant models for GC & LC platforms
- Examine platform transferability for semi-quant models
- Apply models to existing data (products & media)
- Develop pipeline from ToxCast AC₅₀ (or other NAM-based hazard metrics) to lower bound media conc.
- Incorporate into EPA NTA WebApp

Contributing Researchers



This work was supported, in part, by ORD's Pathfinder Innovation Program (PIP) and an ORD EMVL award



Credit: the Research Triangle Foundation

EPA ORD

Seth Newton
Jon Sobus
Hannah Liberatore
Hussein Al-Ghoul*
Alex Chao*
Jarod Grossman*
Kristin Isaacs
Sarah Laughlin*
Charles Lowe
James McCord
Kelsey Miller
Jeff Minucci
Katherine Phillips
Allison Phillips*
Tom Purucker
Randolph Singh*
Mark Strynar
Elin Ulrich
Nelson Yeung*

EPA ORD (cont.)

Kathie Dionisio
Chris Grulke
Kamel Mansouri*
Andrew McEachran*
Ann Richard
Adam Swank
John Wambaugh
Antony Williams

Agilent

Jarod Grossman
Andrew McEachran

GDIT

Ilya Balabin
Tom Transue
Tommy Cathey

* = ORISE/ORAU



Questions?

Groff.Louis@epa.gov



The views expressed in this presentation are those of the author and do not necessarily represent the views or policies of the U.S. Environmental Protection Agency.